



ware Version: 4.1<2F12>

Sample Name :

Time : 19/02/09 05:13 PM

Sample Number:

Study :

Operator :

Document : AUTOSYS_-_0:A

Channel : A

A/D mV Range : 1000

Amplifier : NONE

Vial : 18176/0

Interface Serial # : NONE Data Acquisition Time: 19/02/09 03:47 PM

Time : 0.00 min.

Time : 3.00 min.

Sampling Rate : 1.5625 pts/sec

Data File : C:\TC4\DATA\AOH_014E.RAW

Raw File : C:\TC4\DATA\AOH_007E.RST

Method : C:\TC4\DATA\AOH from C:\TC4\DATA\AOH_007E.RST

Method : C:\TC4\DATA\AOH from C:\TC4\DATA\AOH_007E.RST

Method : C:\TC4\DATA\AOH from C:\TC4\DATA\AOH_007E.RST

Sequence File : C:\TC4\DATA\AOH.SEQ

Sample Volume : 1.0000 uL

Area Reject : 0.000000

Sample Amount : 1.0000

Dilution Factor : 1.00

DEFAULT REPORT

Time [min]	Area [μV·s]	Height [μV]	Area [%]	Norm. Area [%]	BL	Area/Height [s]
0.074	43.64	14.79	0.17	0.00	BB	2.95
0.216	19.78	11.27	0.08	0.00	BB	1.75
0.396	17.35	9.37	0.07	0.00	BV	1.85
0.456	24.74	12.28	0.10	0.00	VV	2.01
0.521	22.75	10.48	0.09	0.00	VB	2.17
0.614	21.42	9.03	0.09	0.00	BB	2.37
0.747	24.36	15.20	0.10	0.00	BB	1.60
1.129	8.39	7.06	0.03	0.00	BB	1.19
1.23	22.58	7.50	0.09	0.00	BV	3.01
1.33	44.79	12.98	0.18	0.00	VB	3.45
1.41	16.85	8.00	0.07	0.00	BB	2.11
1.56	11.97	5.76	0.05	0.00	BB	2.08
1.74	11.62	7.59	0.05	0.00	BV	1.53
1.86	194.21	170.44	0.78	0.00	VB	1.14
2.09	10.29	6.08	0.04	0.00	BB	1.69
2.21	9.48	6.14	0.04	0.00	BB	1.54
2.45	24550.42	2996.79	97.96	0.00	BB	9.18

Missing Component Report
Expedited Retention Time Report
Component

Result File : AOH_007E.RST, Printed on 19/02/09 05:12 PM


Chromatogram

In Name :
 Name : C:\TC4\DATA\ACM_013D.RAW
 ed :
 Time : 0.00 min
 Factor: 0.0

End Time : 3.00 min
 Plot Offset: 0 mV

Sample #: 1
 Date : 19/02/09 05:15 PM
 Time of Injection: 19/02/09 04:28 PM
 Low Point : 4.79 mV
 Plot Scale: 3.5 mV
 High Point : 6.34 mV

Page 1 of 1

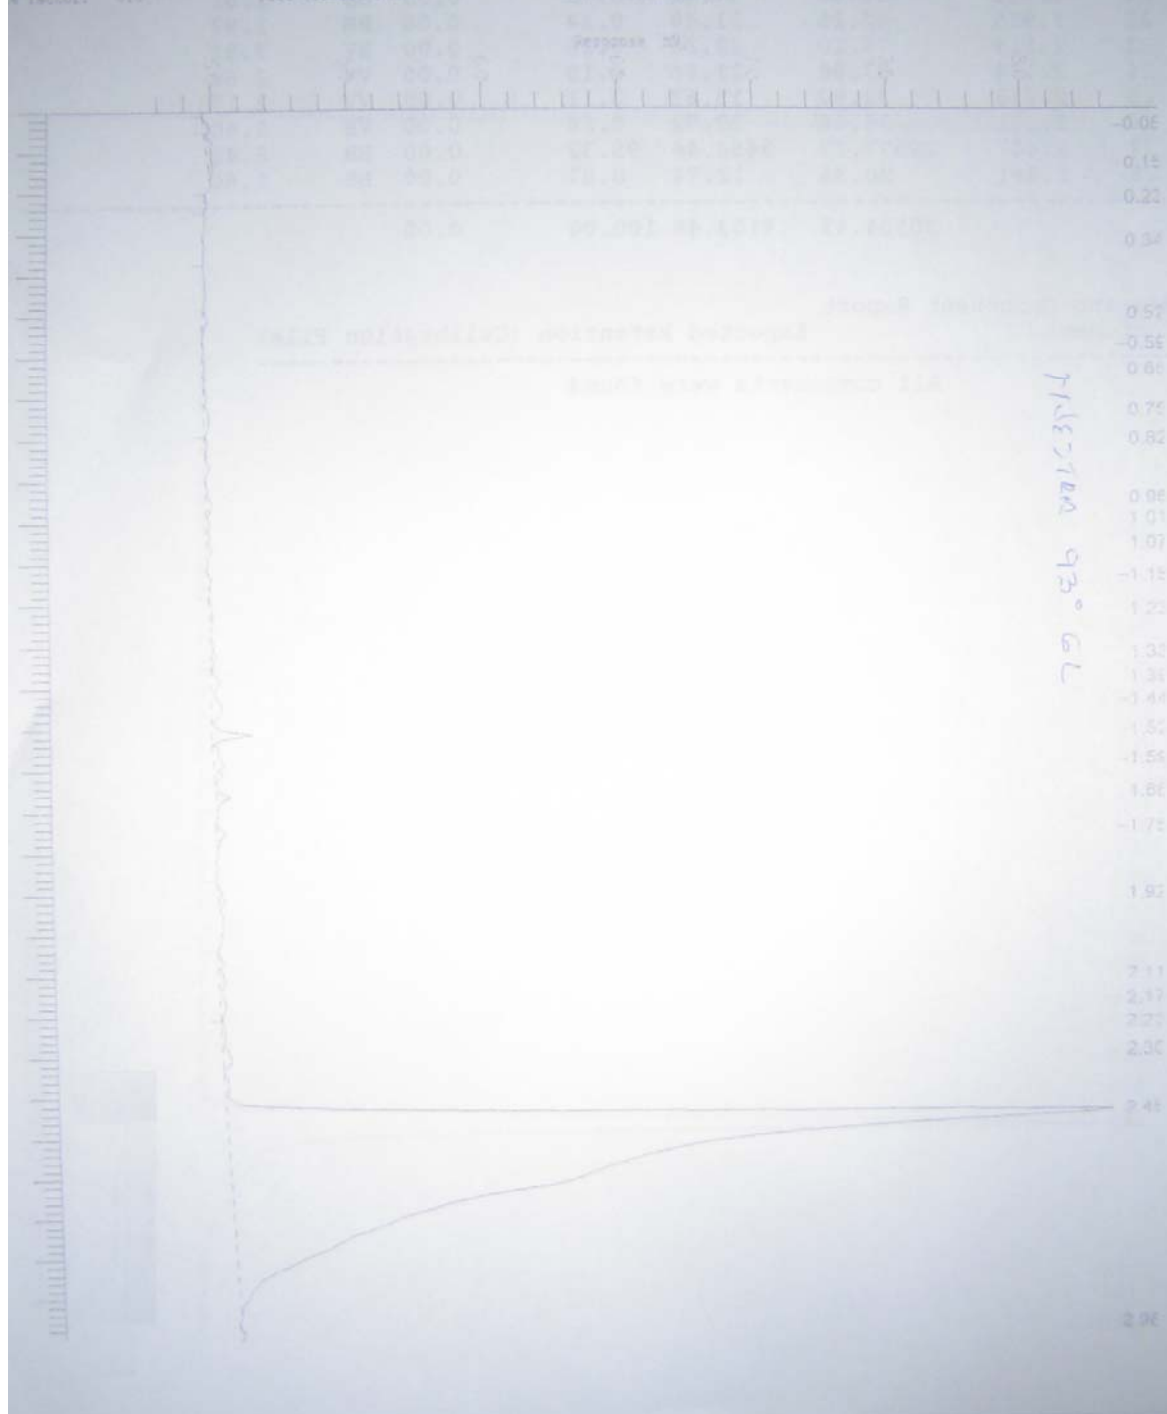

Time min]	Area [$\mu\text{V}\cdot\text{s}$]	Height [μV]	Area [%]	Norm. Area [%]	BL	Area/Height [s]
1.751	56.61	37.42	0.19	0.00	BB	1.51
1.915	42.25	21.48	0.14	0.00	BB	1.97
2.114	78.10	22.26	0.26	0.00	BV	3.51
2.174	57.98	21.66	0.19	0.00	VV	2.68
2.233	33.90	15.63	0.11	0.00	VV	2.17
2.301	78.66	32.72	0.26	0.00	VB	2.40
2.447	29077.27	3454.48	95.32	0.00	BB	8.42
2.981	20.36	12.74	0.07	0.00	BB	1.60
<hr/>						
	30504.43	4153.48	100.00	0.00		

Component Report
nt Expected Retention (Calibration File)

All components were found

Chromatogram

File Name : C:\TC4\DATA\AOM_0063.RAW

Sample #:

Page 1 of 1

Date : 19/02/09 05:01 PM

Time of Injection: 19/02/09 03:09 PM

Start Time : 0.00 min

End Time : 3.00 min


Low Point : 8.47 mV

High Point : 13.96 mV

Gain Factor: 0.0

Plot Offset: 4 mV

Plot Scale: 9.5 mV

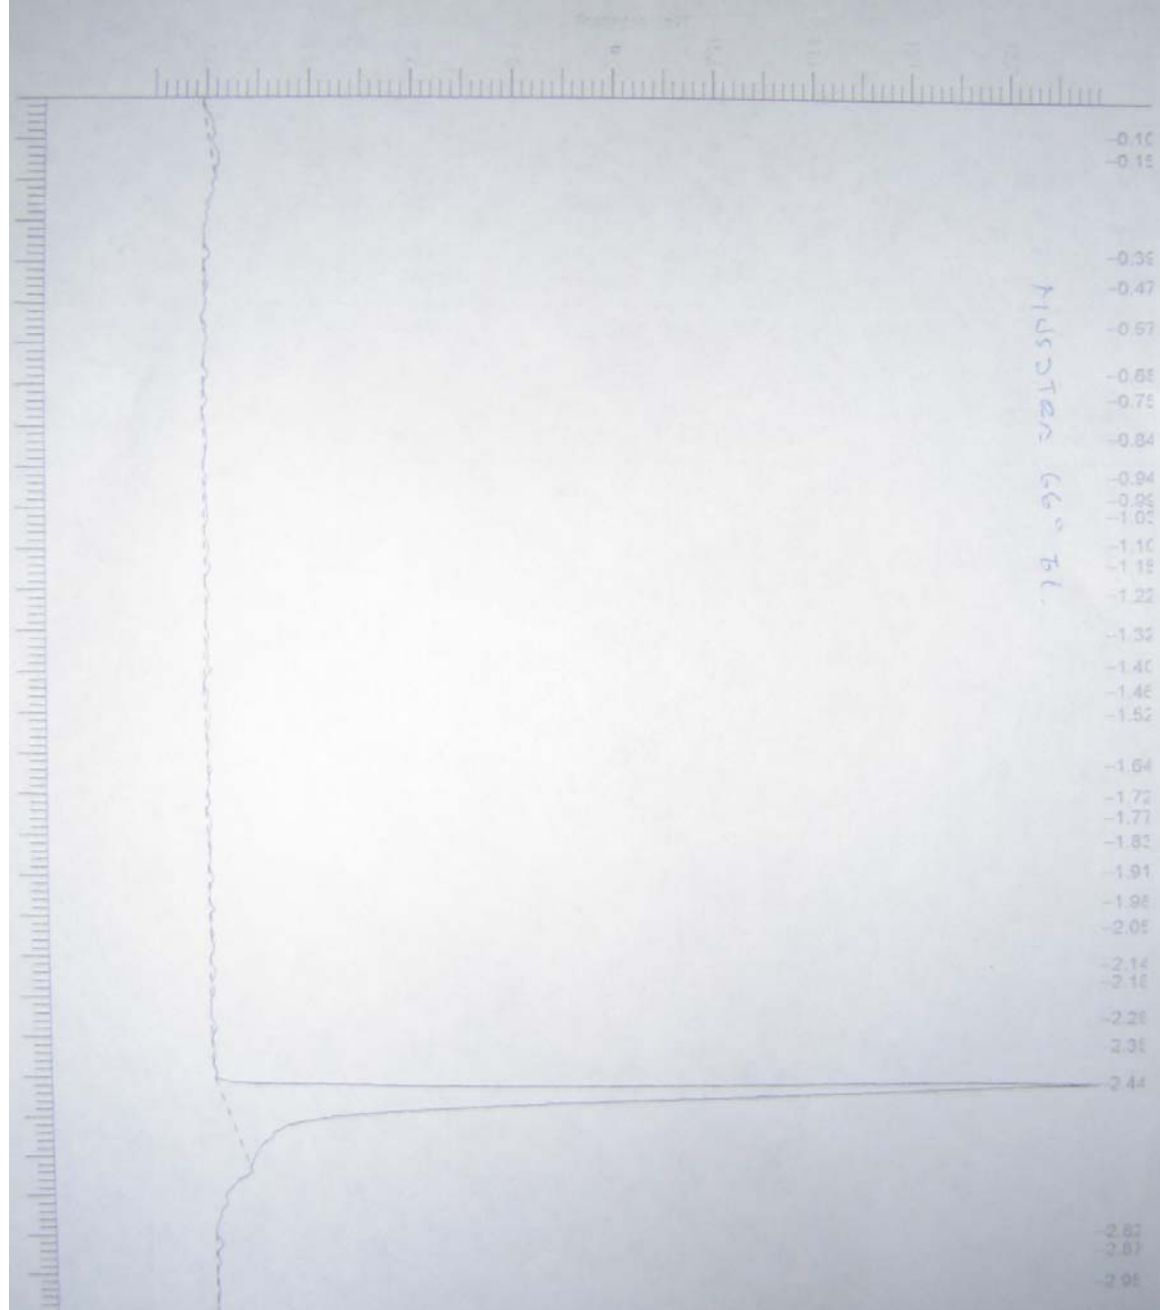

Peak #	Time [min]	Area [pV·s]	Height [pV]	Area [%]	Norm. Area [%]	Area BL	Area/Height [s]
21	1.771	109.66	39.01	0.40	0.00	BV	2.81
22	1.831	36.66	22.73	0.13	0.00	VB	1.61
23	1.908	95.04	51.95	0.34	0.00	BV	1.83
24	1.983	42.57	50.68	0.15	0.00	VB	0.84
25	2.047	50.50	33.68	0.18	0.00	BB	1.50
26	2.140	119.88	55.87	0.43	0.00	BV	2.15
27	2.184	55.47	38.18	0.20	0.00	VB	1.45
28	2.276	90.89	46.84	0.33	0.00	BB	1.94
29	2.346	61.59	37.71	0.22	0.00	BB	1.63
30	2.442	24542.81	8879.34	89.05	0.00	BB	2.76
31	2.819	104.83	73.70	0.38	0.00	BV	1.42
32	2.867	58.42	38.66	0.21	0.00	VV	1.51
33	2.951	69.40	24.46	0.25	0.00	VB	2.84
		27560.46	10351.85	100.00	0.00		

Missing Component Report

Component

Expected Retention (Calibration File)

All components were found